
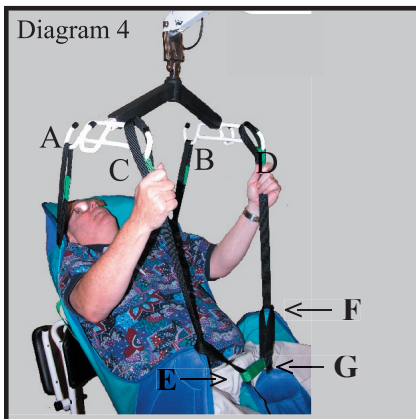
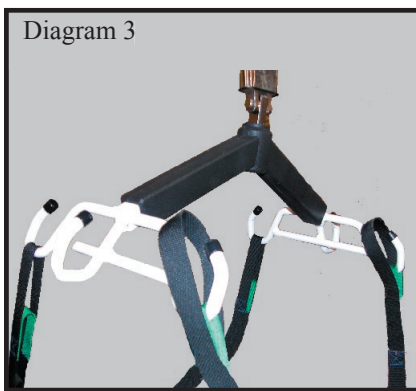
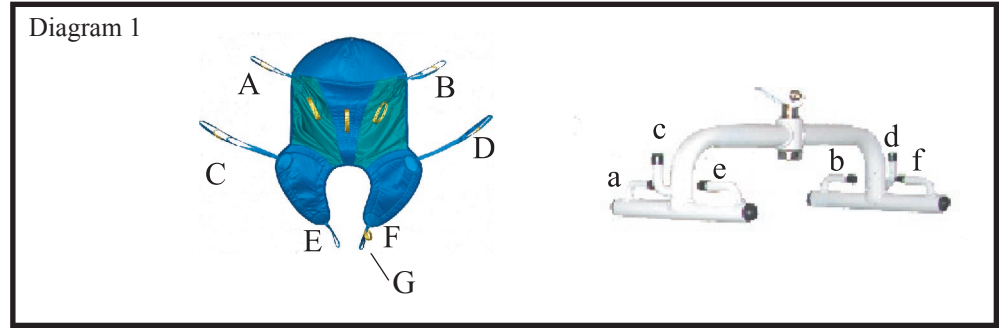


# Apexlift Sling User Guide

## HAMMOCK SLINGS

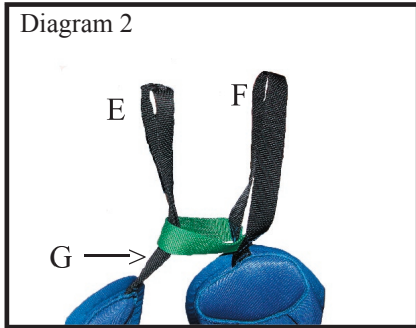

### WARNING!

Step 1: Check sling weight capacity for the patient being lifted. Do not exceed maximum safe working load.

Step 2: Review following procedures carefully prior to attempting lift. Call with any questions.

Step 3: Position the sling under and behind the back with color adjustment strap on outside. A & B should be at shoulder height.

Step 4: Pull the leg straps E & F down behind patient, and between legs as in Diagram 4.

Step 5: Hook E & F through small loop G as in Diagram 2.


Step 6: Slip the ends of C & D through E & F (ends of loops) and hook to spreader bar at e & f as in Diagram 4.

Step 7: Do not lock caster brakes to allow lift to properly balance weight.

Step 8: Proceed with lift and transfer as in Diagram 5.

#### SLING LOOP OPTIONS

Long Loop- reclined position.  
Center Loop- semi-reclined position  
Short Loop- most upright position

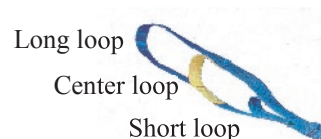

SEE REVERSE FOR ADDITIONAL SLING OPTIONS