



BestSling User Guide

INVACARE COMPATIBLE SLINGS

Diagram 1

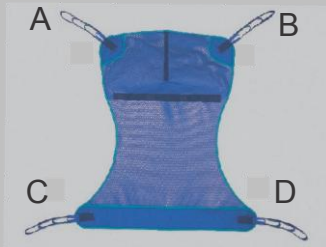

WARNING!

Diagram 2




Step 1: Check sling weight capacity for the patient being lifted. Do not exceed maximum safe working load.

Step 2: Review following procedures carefully prior to attempting lift. Call with any question.

Step 3: Position the sling under and behind the back with the color adjustment strap on outside. A & B should be draped over the shoulders as in Diagram 2.

Step 4: Carefully, with help from another caregiver, if needed, pull the sling portion C & D forward to the bend of the knee as in Diagram 2.

Diagram 3

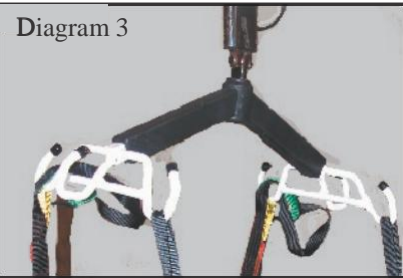


Step 5: Hook Loops A & B on sling to A & B on the spreader bar as in Diagram 3.

Step 6: Hook loops C & D on sling to C & D on spreader bar as in Diagram 3.

Step 7: Do not lock caster brakes to allow lift to properly balance weight.


Diagram 4

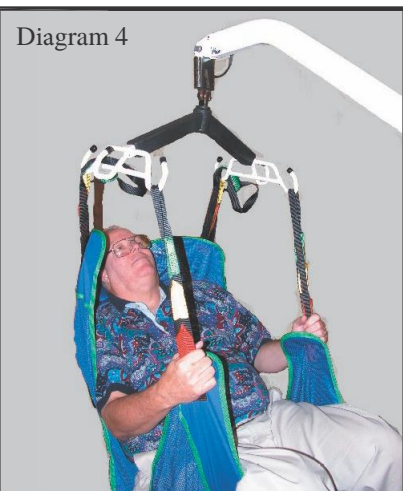

Step 8: Proceed with lift and transfer as in Diagram 4.

SLING LOOP OPTIONS

Long Loop- reclined position.
Center Loop- semi-reclined position
Short Loop- most upright position

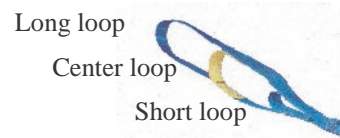

1-877-822-9033

INVACARE is a registered trademark of INVACARE CORPORATION