
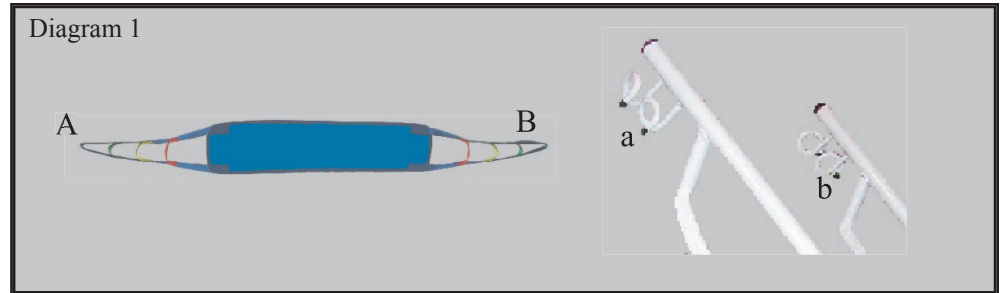


BestSling User Guide

BUTTOCK STRAP

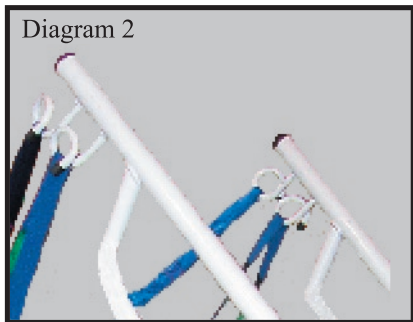

WARNING!

Step 1: Check sling weight capacity for the patient being lifted. Do not exceed maximum safe working load.

Step 2: Review following procedures carefully prior to attempting lift. Call with any questions.

Step 3: Position the sling around the buttocks of the patient. This sling is designed to support the middle and lower part of the body.

Step 4: Attach the sling strap on the lower “pig tail” “A” on the mast of the Stella Stand Assist lift as in Diagram 1. Bring the other side around the back of the patient’s buttocks (to fit like a park swing) and attach to lower “pig tail” “B”.

Step 5: Position sling so it gives the greatest support to middle and lower part of patient being lifted.

Step 6: Notice, in Diagram 2, that the Buttock Strap must be used with the Stand Assist Sling. These slings are designed to compliment one another in providing the greatest comfort and security for the patient being transferred.

Step 7: Do not lock caster brakes to allow lift to properly balance weight.

Step 8: Proceed with lift and transfer as in Diagram 3.

NOTE: It is not uncommon for the strap to loosen and drop down as lift proceeds.